



STRUCTURAL ENGINEERING DIVISION
Test Floor Laboratory
Department of Civil Engineering
University of Engineering and Technology Lahore, 54890
Pakistan. Ph: 92-42-99029202

Ref: CED/TFL/04/1334

Dated: 26-04-2022

Dated of Test: 29-04-2022

To

M/S Precast Building System
Lahore


Subject: - **CALIBRATION OF DYNAMOMETER (MARK: TFL/04/1334)** (Page -1/1)

Ref: Your letter No. P-4(A)/12/2022, dated: 25/04/2022 on the subject cited above. One Dynamometer as received by us has been calibrated. The results are tabulated as under:

Total Range : Zero - 5000 (kg)
Calibrated Range : Zero - 4000 (kg)

Dynamometer Readings (kg)	500	1000	1500	2000	2500	3000	3500	4000
Calibrated Readings (kg)	330	800	1160	1660	2250	2620	3100	3510

Calibration Curve for Dynamometer

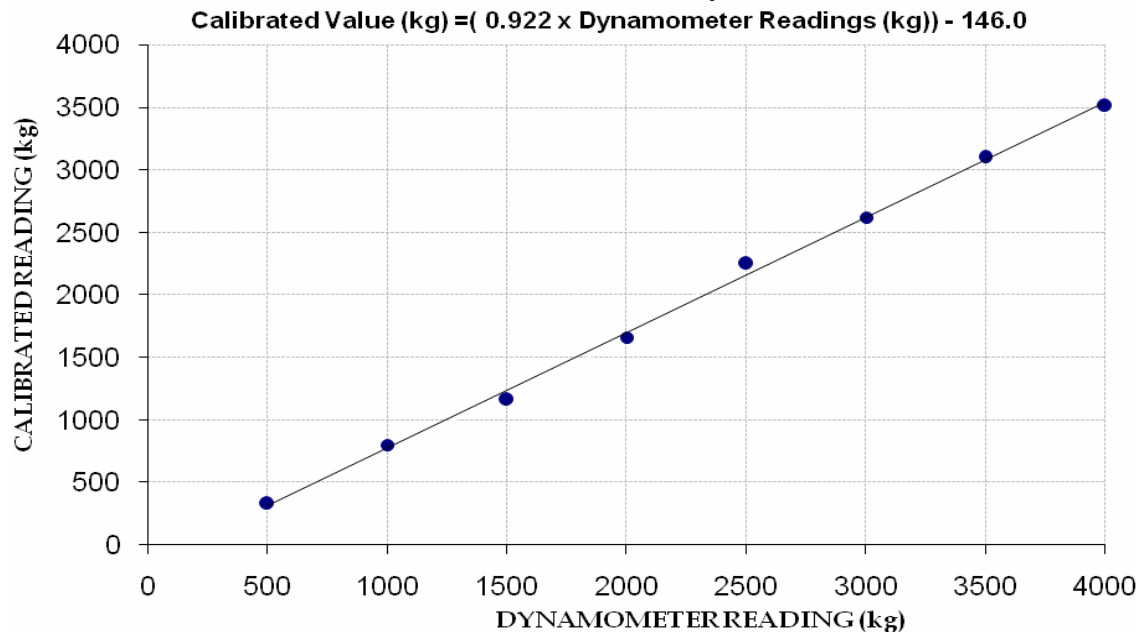

I/C Testing Laboratoires
UET Lahore, Pakistan.

Note:

- 1- You can See your reports On Internet in the following web site
http://www.uet.edu.pk/faculties/facultiesinfo/civil/index.html?RID=testing_reports
- 2- The above results pertain to sample /samples supplied to this laboratory.
- 3- Sealed sample / Unsealed sample / Marked sample/Signed Samples



STRUCTURAL ENGINEERING DIVISION
Test Floor Laboratory
Department of Civil Engineering
University of Engineering and Technology Lahore, 54890
Pakistan. Ph: 92-42-99029202

To,
 Resident Engineer
 NESPAK

Construction of Underpass at Ghulab Devi Hospital and Additional Lanes on Lahore Bridge

Reference # CED/TFL **1353** (Enr. Amina Rajput)
 Reference of the request letter # 3772/103/GD/RE/05/243

Dated: 28-04-2022
 Dated: 07-04-2022

Tension Test Report (Page -1/1)

Date of Test 29-04-2022
 Gauge length 8 inches
 Description Deformed Steel Bar Tensile and Bend Test as per ASTM-A615

Sr. No.	Weight (lbs/ft)	Diameter/ Size		Area (in ²)		Yield load (kg)	Breaking Load (kg)	Yield Stress (psi)		Ultimate Stress (psi)		Elongation (inch)	% Elongation	Remarks
		Nominal (#)	Actual (inch)	Nominal	Actual			Nominal	Actual	Nominal	Actual			
1	0.362	3	0.368	0.11	0.106	3100	4600	62200	64220	92200	95300	1.20	15.0	Batala Premium
2	0.360	3	0.367	0.11	0.106	3000	4600	60200	62450	92200	95800	1.10	13.8	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
Note: only two samples for tensile and one sample for bend test														
Bend Test														
#3 Bar Bend Test Through 180° is Satisfactory														

I/C Testing Laboratoires
UET Lahore, Pakistan.

Note:

- 1- You can See your reports On Internet in the following web site
http://www.uet.edu.pk/faculties/facultiesinfo/civil/index.html?RID=testing_reports
2. The above results pertain to sample /samples supplied to this laboratory.
- 3- Sealed sample / Unsealed sample / Marked sample/Signed Samples



STRUCTURAL ENGINEERING DIVISION
Test Floor Laboratory
Department of Civil Engineering
University of Engineering and Technology Lahore, 54890
Pakistan. Ph: 92-42-99029202

To,
Senior Project Manager
Shifa Development Services
Shifa National Hospital, Lahore Sheikhpura Road, Faisalabad

Reference # CED/TFL **1354** (Enr. Amina Rajput)
Reference of the request letter # SNHF/SDS/ST/02

Dated: 28-04-2022
Dated: 28-04-2022

Tension Test Report (Page -1/1)

Date of Test 29-04-2022
Gauge length 8 inches
Description Deformed Steel Bar Tensile and Bend Test as per ASTM-A615

Sr. No.	Weight (lbs/ft)	Diameter/ Size (inch)		Area (in ²)		Yield load (kg)	Breaking Load (kg)	Yield Stress (psi)		Ultimate Stress (psi)		Elongation (inch)	% Elongation	Remarks
		Nominal	Actual	Nominal	Actual			Nominal	Actual	Nominal	Actual			
1	0.373	3/8	0.374	0.11	0.110	3600	5100	72200	72340	102200	102500	1.10	13.8	Kamran Steel
2	0.377	3/8	0.376	0.11	0.111	3500	5100	70200	69640	102200	101500	1.00	12.5	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
Note: only two samples for tensile and one sample for bend test														
Bend Test														
3/8" Dia Bar Bend Test Through 180° is Satisfactory														

I/C Testing Laboratoires
UET Lahore, Pakistan.

Note:

- 1- You can See your reports On Internet in the following web site
http://www.uet.edu.pk/faculties/facultiesinfo/civil/index.html?RID=testing_reports
- 2- The above results pertain to sample /samples supplied to this laboratory.
- 3- Sealed sample / Unsealed sample / Marked sample/Signed Samples



STRUCTURAL ENGINEERING DIVISION
Test Floor Laboratory
Department of Civil Engineering
University of Engineering and Technology Lahore, 54890
Pakistan. Ph: 92-42-99029202

To,
 Sub Divisional Officer
 Buildings Sub Division
 Bahawalnagar
 (Construction of Circuit House at District Bahawalpur)

Reference # CED/TFL **1355** (Enr. Amina Rajput)
 Reference of the request letter # 496/BWN

Dated: 28-04-2022
 Dated: 24-03-2022

Tension Test Report (Page -1/1)

Date of Test 29-04-2022
 Gauge length 8 inches
 Description Deformed Steel Bar Tensile and Bend Test as per ASTM-A615

Sr. No.	Weight (lbs/ft)	Diameter/ Size (inch)		Area (in ²)		Yield load (kg)	Breaking Load (kg)	Yield Stress (psi)		Ultimate Stress (psi)		Elongation (inch)	% Elongation	Remarks
		Nominal	Actual	Nominal	Actual			Nominal	Actual	Nominal	Actual			
1	0.404	3/8	0.389	0.11	0.119	3800	5100	76200	70510	102200	94700	1.20	15.0	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
Note: only one sample for tensile and one sample for bend test														
Bend Test														
3/8" Dia Bar Bend Test Through 180° is Satisfactory														

I/C Testing Laboratoires
UET Lahore, Pakistan.

Note:

- 1- You can See your reports On Internet in the following web site
http://www.uet.edu.pk/faculties/facultiesinfo/civil/index.html?RID=testing_reports
- 2- The above results pertain to sample /samples supplied to this laboratory.
- 3- Sealed sample / Unsealed sample / Marked sample/Signed Samples



STRUCTURAL ENGINEERING DIVISION
Test Floor Laboratory
Department of Civil Engineering
University of Engineering and Technology Lahore, 54890
Pakistan. Ph: 92-42-99029202

To,
 Sub Divisional Officer
 Buildings Sub Division
 Fort Abbas
 (Construction of Police Station Fort Abbas)

Reference # CED/TFL **1356** (Enr. Amina Rajput)
 Reference of the request letter # 54

Dated: 28-04-2022
 Dated: 01-04-2022

Tension Test Report (Page -1/1)

Date of Test 29-04-2022
 Gauge length 8 inches
 Description Deformed Steel Bar Tensile and Bend Test as per ASTM-A615

Sr. No.	Weight (lbs/ft)	Diameter/ Size (inch)		Area (in ²)		Yield load (kg)	Breaking Load (kg)	Yield Stress (psi)		Ultimate Stress (psi)		Elongation (inch)	% Elongation	Remarks
		Nominal	Actual	Nominal	Actual			Nominal	Actual	Nominal	Actual			
1	0.408	3/8	0.391	0.11	0.120	3600	4900	72200	66220	98200	90200	1.20	15.0	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	-	-	-	-	
Note: only one sample for tensile and one sample for bend test														
Bend Test														
3/8" Dia Bar Bend Test Through 180° is Satisfactory														

I/C Testing Laboratoires
UET Lahore, Pakistan.

Note:

- 1- You can See your reports On Internet in the following web site
http://www.uet.edu.pk/faculties/facultiesinfo/civil/index.html?RID=testing_reports
- 2- The above results pertain to sample /samples supplied to this laboratory.
- 3- Sealed sample / Unsealed sample / Marked sample/Signed Samples



STRUCTURAL ENGINEERING DIVISION
Test Floor Laboratory
Department of Civil Engineering
University of Engineering and Technology Lahore, 54890
Pakistan. Ph: 92-42-99029202

I/C Testing Laboratories
UET Lahore, Pakistan.

Note:

- 1- You can See your reports On Internet in the following web site
http://www.uet.edu.pk/faculties/facultiesinfo/civil/index.html?RID=testing_reports
2. The above results pertain to sample /samples supplied to this laboratory.
- 3- Sealed sample / Unsealed sample / Marked sample/Signed Samples